biophotas

cellumaRx

User Manual

DOC-0001 Rev. G, January 2013

Table of Contents

Intended Use and Device Description_____3

Important Safety Instructions _____ 4

Preparing the Celluma® for Use _____ 6

Celluma – Protocols for Use _____7

Celluma - Instructions for Use _____7

Caring for Your Celluma _____10

Useful Tips and Frequently Asked Questions _____ 10

Technical Support _____ 11

Intended Use:

The Biophotas Celluma® device is intended to deliver heat in the IR spectrum to provide topical heating for the purpose of elevating tissue temperature; for the temporary relief of minor muscle and joint pain, arthritis and muscle spasm; relieving stiffness; promoting the relaxation of muscle tissue; and to temporarily increase local blood circulation. The blue spectrum is intended to reduce mild to moderate acne vulgaris.

Device Description:

The Celluma® is a lightweight device which uses specific wavelengths of light, produced by light emitting diodes (LEDs), to manage aesthetic conditions. Celluma produces light in the near infrared region of the spectrum (880 nm) intended to provide topical heating to tissue. Blue light (464 nm) is intended to help reduce the appearance of mild to moderate acne.

Contraindications:

There are no known contraindications at the present time.

Important Safety Instructions

Read all instructions before using this device. Save these instructions for future reference.

This manual contains important safety symbols and instructions. Please pay attention to these symbols and follow all instructions given.

General Warning or Caution

The Exclamation Symbol in the figure above appears in Warning and Caution statements in this document. This symbol designates an area where personal injury or damage to the equipment is possible.

Electric Shock Symbol

The Electrical Shock Symbol in the figure above appears throughout this manual. This symbol indicates a hazard arising from dangerous voltage. Any mishandling could result in irreparable damage to the equipment, and personal injury or death.

Protective Conductor Terminal Symbol

The protective conductor terminal symbol in the above figure identifies the location of the bonding terminal, which is bonded to conductive accessible parts of the enclosure for safety purposes.

~ *Alternating voltage symbol*

This international symbol implies an alternating voltage or current.

 *Fuses Symbol*

The fuse symbol in the figure above identifies the fuse location on the Celluma.

| *On Symbol*

The On Symbol in the figure above represents a power switch position on the Celluma. This symbol represents a Power On condition.

O *Off Symbol*

The Off Symbol in the figure above represents a power switch position on the Celluma. This symbol represents a Power Off condition.

Waste Electrical and Electronic Equipment (WEEE)

WEEE Directive Symbol

This symbol on the product or on its packaging indicates that this product must not be disposed of with regular waste. Instead, it is the user responsibility to dispose of waste equipment according to the local laws. For information about where the user can drop off the waste equipment for recycling, please contact your local BioPhotas, Inc. representative.

Celluma® Product Safety Information

1. Read and keep these instructions.
2. Follow instructions and heed all warnings. Install in accordance with the manufacturer's instructions.
3. Make sure that the Power Cord is unplugged from wall outlet before cleaning the apparatus.
4. Do not use this device near water.
5. Do not use this device near strong sources of electromagnetic radiation. Device may inadvertently shut off when operated in the presence of a high electromagnetic field.
6. Do not use volatile solvents (such as toluene, alcohol, etc.) to clean the device. Such solvents may damage the housing and control surface.
7. Clean with a soft dry cloth.
8. If the housing or control surface is seriously contaminated, use a soft cloth moistened with a non-alcohol disinfectant to clean the device.
   Wring out cloth before cleaning to prevent any fluid from penetrating into the housing. Wipe the device with a clean, dry cloth after cleaning.
9. Do not install near any heat source such as radiators, heat registers, stoves or other apparatus that produce heat.
10. Protect the power cord from being walked on or pinched particularly at plugs, convenience receptacles, or matted with extension cord or the point where they exit from the device.
11. Only use attachments/accessories specified by the manufacturer.
12. Unplug this apparatus during lightning storms or when unused for long periods of time.
13. There are no user-serviceable parts inside this device. Refer all servicing to the manufacturer.
14. Servicing is required when the apparatus has been damaged in any way, such as when the power cord is damaged, liquid has been spilled or objects have fallen into the apparatus or the apparatus has been exposed to rain or if the apparatus does not operate normally or has been dropped.
15. Operating and Storage Temperatures : 3 ~ 35°C, Relative Humidity: 10~80% (non-condensing)
16. Do not fold, crease or crimp the Celluma beyond its design capabilities. When shaping the device around a body part - such as an arm - the inward curve should not be smaller than 6" in diameter. When bending the device convexly (lights facing outwards) the curve should not be less than 16" in diameter.

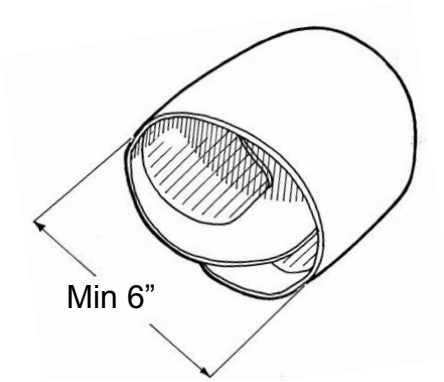

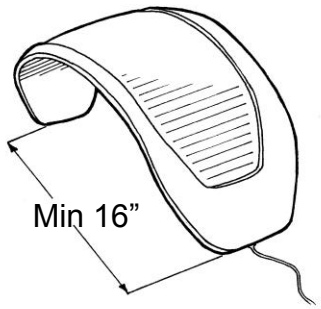

Preparing the Celluma® for Use:

Inspect for Damage

The Celluma is carefully packaged at the factory to minimize the possibility of damage during shipping. Inspect the box for external signs of damage or mishandling. Inspect the contents for damage. If there is visible damage to the instrument upon receipt, inform the shipping company and Biophotas immediately.

	WARNING Do not attempt to operate this equipment if there is evidence of shipping damage or you suspect the unit is damaged. Damaged equipment may present additional hazards to you. Contact technical support for advice before attempting to plug in and operate damaged equipment.

	WARNING Only authorized personnel may service this equipment. See manual for safety information.

BIOPHOTAS, INC.
250 EL CAMINO REAL
SUITE 110
TUSTIN, CA 92780
(714) 838 1956
www.biophotas.com

Celluma® – Protocols for Use

NOTE: ***When making changes to your health and wellness routine, it may be advisable to consult with your physician before proceeding***

Programs

When should I use "Acne"? Use the Celluma Acne program at the first signs of acne breakout. The treatment consists of 8 treatment sessions spread over 4 weeks, allowing 2 treatments per week, once every three days.

When should I use "Aches & Pains"? Use the Aches & Pains mode for management and temporary relief of minor muscle and joint pain, stiffness, minor arthritis pain or muscle spasms and to provide a temporary increase in local blood circulation. Do this once every three days.

Suggested Product Positioning

Celluma®: Instructions for Use:

Product Assembly

1. Connect the power supply to the Celluma console by inserting the end of the power connector into the side of the console.
2. Insert the power supply into an electrical outlet. The perimeter lights on the console will illuminate and circle twice.

User Preparation

1. Assure that the user is properly positioned and the skin area to be treated is clean and dry. Make-up and other cosmetics should be removed. Many formulas contain minerals which can deflect the light and reduce energy absorption.
2. For best results, the Celluma should be positioned in close proximity to bare skin. Place the Celluma so that the light panel is no more than 1 inch (or as close as possible without touching) the skin.
3. Use the iGoggles provided with Celluma.

iGoggles™

Do not lie upon or lean against the Celluma. The Celluma is not designed to withstand full body weight or extreme pressure.

Failure to follow this precaution could result in shock!

When making changes to your health and wellness routines it may be advisable to consult with your physician before proceeding.

Healthcare providers (doctors, nurses, estheticians, etc.) as well as patients should avoid looking directly into the light. Patients should wear eye protection during the treatment.

Do not use if the patient is pregnant or breastfeeding.

Do not use if the patient or administrator has epilepsy.

Avoid using when the patient is taking cortisone injections or any other kind of steroid injection(s).

Perform a 90 second "patch test" on a non-visible area of the skin prior to any new facial or body treatment. If any adverse reactions occur, discontinue any further use of the system.

Do not look directly at the light, and wear the iGoggles provided or use appropriate eye protection.

Select and Begin a Celluma Program

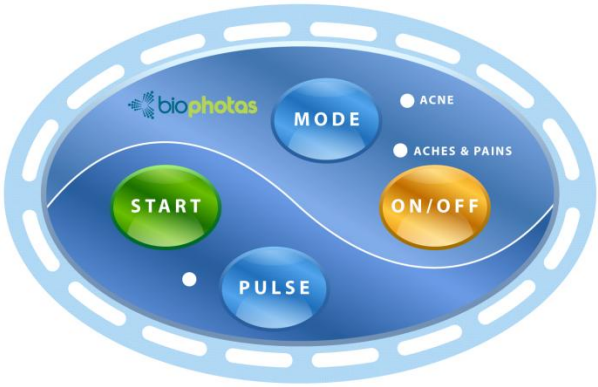

1. To begin a Celluma session, press the ON/OFF button. The device automatically defaults to the Acne program as indicated by the flashing blue light. Then depress the MODE button to select the desired program, if not Acne. Once a program is selected, the corresponding light and perimeter lights will turn on.
2. The Celluma may be used in either Pulse mode or without Pulse mode. Pulse mode causes pulsing lights. Each time the Celluma is turned on it defaults to the Pulse mode as shown by the amber light. To switch from Pulse mode, simply press the PULSE button once. The device will now run without the Pulse mode and the amber light will go off. To return to Pulse mode, press the PULSE button again. Selection of either mode is based on personal preference. If for any reason you are uncomfortable with the pulsing lights, switch Pulse mode off.
3. With the Celluma in position, press the START button to begin the selected program. The corresponding indicator light will stay lit. Illumination will increase slowly over the first 20 seconds, and remain steady.
4. All programs run for 30 minutes and may be stopped by pressing the ON/OFF button. At the end of the program, the illumination will slowly decrease and the device will automatically switch off. If a program is interrupted, re-select the desired program and press the START button to begin over. For best results use the Celluma for a full 30 minutes. The Celluma may be used on the same area once every three days.

Caring for Your Celluma®

The Celluma is protected with a stain and water-repellant material that is applied to the fabric portion of the device. If your Celluma requires spot cleaning, carefully follow the instructions below.

1. Do not use volatile solvents (such as toluene, alcohol, etc.) to clean the device. Such solvents may damage the housing and control surface.
2. Clean with a soft dry cloth.
3. If the console surface is seriously contaminated, use a soft cloth moistened with a non-alcohol based disinfectant to clean the device. Wring out cloth before cleaning to prevent any fluid from penetrating into the housing. Wipe the device with a clean, dry cloth after cleaning.

Disposable hygienic barrier sleeves are available in Packs of 100 and may be purchased by contacting BioPhotas Customer Care at 1 (714) 838 1956 or visiting www.biophotas.com to place your order.

Useful Tips and Frequently Asked Questions

Q: What is the intended use of the Celluma?
A: The Biophotas Celluma® device is intended to deliver heat in the IR spectrum to provide topical heating for the purpose of elevating tissue temperature; for the temporary relief of minor muscle and joint pain, arthritis and muscle spasm; relieving stiffness; promoting the relaxation of muscle tissue; and to temporarily increase local blood circulation. The blue spectrum is intended to reduce inflammatory acne vulgaris.

Q: Does the Celluma utilize UV light?
A: No.

Q: How long does a Celluma treatment session last?
A: 30 minutes.

Q: Are there any special preparations required before using the Celluma?
The Celluma should be in close proximity with the skin that should be free of clothing, make-up, or anything else which may deflect the light away from the skin, while not actually touching the skin. Do not look directly at the light, and wear the iGoggles provided or use appropriate eye protection.

Q: Why is it recommended to remove make-up?
A: Many make-up formulas contain minerals that may deflect the light. Clean, freshly washed skin is recommended for best results. Perform a 90 second "patch test" on a non-visible area of the skin prior to any new facial or body treatment. If any adverse reactions occur, discontinue any further use of the system.

Q: How close should the Celluma be placed to the skin?
A: Position the Celluma as close to your skin as possible, ideally one inch, but without making skin contact. Do not look directly into the light, and protect your eyes with the iGoggles provided with the Celluma, or use other appropriate eye protection.

Q: Can I travel with the Celluma?
A: Yes. Celluma is lightweight and portable making it ideal for travel to or from the office or gym. For travel outside of the U.S. be sure to check for correct power source and electrical input.

Q: What should I do if I cannot use the Celluma?
A: If there is a medical problem, please contact your doctor. If there is a technical problem with the Celluma, please call BioPhotas, Inc. at the number listed in Technical Support (following).

Technical Support

If the Celluma will not Power up	• Check plug and electrical socket • If the unit still has no power - call the number below and ask for support.
If Celluma does not respond to controls	• First turn the main power switch off • Wait five seconds • Then switch back on • If the problem persists call the number below and ask for support.
For additional issues	• Call the number below and ask for support.

Contact Information

Biophotas, Inc.

250 EL CAMINO REAL
SUITE 110
TUSTIN, CA 92780

Telephone: (714) 838 – 1956
Fax: (714) 838 – 1447
E-mail: info@biophotas.com
Web Site: www.biophotas.com

Only authorized personnel may service this equipment. See manual for safety information.